

Steady-State Movement Related Potentials for Brain–Computer Interfacing

Kianoush Nazarpour*, *Member, IEEE*, Peter Praamstra, R. Chris Miall, and Saeid Sanei, *Senior Member, IEEE*

Abstract—An approach for brain–computer interfacing (BCI) by analysis of steady-state movement related potentials (ssMRPs) produced during rhythmic finger movements is proposed in this paper. The neurological background of ssMRPs is briefly reviewed. Averaged ssMRPs represent the development of a lateralized rhythmic potential, and the energy of the EEG signals at the finger tapping frequency can be used for single-trial ssMRP classification. The proposed ssMRP-based BCI approach is tested using the classic Fisher’s linear discriminant classifier. Moreover, the influence of the current source density transform on the performance of BCI system is investigated. The averaged correct classification rates (CCRs) as well as averaged information transfer rates (ITRs) for different sliding time windows are reported. Reliable single-trial classification rates of 88%–100% accuracy are achievable at relatively high ITRs. Furthermore, we have been able to achieve CCRs of up to 93% in classification of the ssMRPs recorded during imagined rhythmic finger movements. The merit of this approach is in the application of rhythmic cues for BCI, the relatively simple recording setup, and straightforward computations that make the real-time implementations plausible.

Index Terms—Brain–computer interfacing (BCI), EEG, steady-state movement related potentials (ssMRPs).

I. INTRODUCTION

MOVEMENT related brain activity has been studied for many years by means of readiness potentials (RPs) [1]. The RP is typically recorded during execution of self-paced voluntary movements. The contralaterally dominant part of movement related brain activity preceding movement is called lateralized RP (LRP) [2]. This may be computed by subtraction of slow EEG potentials recorded ipsilaterally to the side of movement from potentials recorded contralaterally, followed by averaging of resultant potentials associated with left and right finger movements [3]. Temporal and spatial characteristics of averaged RPs and LRPs have been well investigated in cognitive and clinical neuroscience studies [1], [4].

Manuscript received September 3, 2008; revised January 26, 2009. First published April 28, 2009; current version published July 15, 2009. This work was supported by the Wellcome Trust, U.K. The work of S. Sanei was supported by The Leverhulme Trust, U.K. *Asterisk indicates corresponding author.*

*K. Nazarpour was with the Centre of Digital Signal Processing, Cardiff University, Cardiff CF24 3AA, U.K. He is now with the Behavioural Brain Sciences Centre, School of Psychology, University of Birmingham, Birmingham B15 2TT, U.K. (e-mail: k.nazarpour@bham.ac.uk).

P. Praamstra and R. C. Miall are with the Behavioural Brain Sciences Centre, School of Psychology, University of Birmingham, Birmingham B15 2TT, U.K. (e-mail: p.praamstra@bham.ac.uk; r.c.miall@bham.ac.uk).

S. Sanei is with the Centre of Digital Signal Processing, School of Engineering, Cardiff University, Cardiff CF24 3AA, U.K. (e-mail: SaeidS@cf.ac.uk).

Color versions of one or more of the figures in this paper are available online at <http://ieeexplore.ieee.org>.

Digital Object Identifier 10.1109/TBME.2009.2021529

Asymmetric RPs during discrete finger movements are readily recordable from almost all subjects [1]. Pioneering studies such as [5], and [6] showed that RP can be detected several hundred milliseconds prior to an overt movement and it was concluded that the asymmetric spatial distribution of these scalp potentials reflects motor preparation for a specific effector. The simple nature of RP signals has made them fairly effective for brain–computer interfacing (BCI) applications [7], [8]. For instance, the Berlin and Tübingen BCI research groups have achieved above 90% correct binary classification rates [7]–[11] by developing various methodological and mathematical techniques. Despite the outstanding BCI performances by means of RPs, the use of such an approach is limited when compared to the P300- and the μ -rhythm-based BCI protocols. There are several issues limiting the applicability of RPs; first, the inevitable dc drifts in EEG measurements due to sweating or electrode displacements, especially if the experiments become lengthy. Second, several low-frequency artifacts such as postural changes, respiration, and dc drifts within short data windows of 0.5 s length before the movement onset reduce the signal (RP) to noise ratio. In addition, after segmenting the recorded EEGs, a baseline removal stage is needed [8]. Although finding a short reference interval can be straightforward in offline analysis, the identification of such a reference interval within the online EEG stream is troublesome in real-time applications. Another problem arises from the nature of the RP: in order to allow the RP build up over time, the intermovement interval should be of several seconds [1]. Recent BCI studies, such as in [8] and [12], have attempted to modify the conventional RP-based BCI paradigms by instructing the subjects to tap at faster paces than usual. The information transfer rate (ITR)—measured in bits per minute (bpm) [13], [14]—was increased. However, faster tapping led to decrement of the correct classification rates (CCRs). For instance, as reported in [12], in binary classification of RP features, the misclassification increased from 5% (ITR \approx 18.6 (bpm)) to 19% (ITR \approx 52.9 (bpm)) when the intertap intervals (ITIs) dropped from 2 to 0.5 s.

An alternative approach for BCI based on steady-state movement related potentials (ssMRPs) is presented here, which overcomes the aforementioned difficulties and provides desirable classification rates in a high-ITR framework. It does not imply any extra computational load, and therefore, its real-time implementation is possible.

This paper is organized as follows. In Section II, we first briefly review the conventional applications of brain steady-state visual evoked potentials (ssVEPs) for BCI. The main motivation and the neurological background of using ssMRPs for BCI

applications are then presented. In Section III, we propose an effective ssMRP recording protocol suitable for real-time BCI applications and explain the two experiments we carried out. Then, the preprocessing, feature extraction, and classifier design stages are described. Section IV reports the results where the spatiotemporal characteristics of the averaged ssMRPs will be presented first. We subsequently report the results of our BCI scheme during the movement initiation and the synchronization states and also during the course of the trials. We further investigate the effect of the time window (TW) size on the BCI performance in Section IV-C. In Section IV-D, we consider the effect of the coexisting transient VEPs on ssMRP measurements. The applicability of ssMRP-based BCI in real-life rehabilitation problems and its extension to motor imagery BCI are then discussed in this section. Moreover, in Section IV-F, we investigate how successful the subjects are in maintaining the correct rhythm when the taps are carried out without the visual cues. Section V presents the concluding remarks.

II. BRAIN STEADY-STATE POTENTIALS FOR BCI

Conventionally, in steady-state potential-based BCI, users are exposed to rhythmic visual or audio cues. For instance, in the increasingly important ssVEPs-based BCI system, bilaterally distributed visually evoked brain potentials are recorded from the visual cortex. Since the fundamental frequency of the stimulation [15], [16] and its first few harmonics [17] are dominant spectral components of the recorded EEG, multiclass BCIs may be realized without extensive subject training [18]. In an ssVEP-based BCI, in order to have an output, the user has to shift their gaze to the flashing stimulation corresponding to the task of interest, and hence, the BCI would be limited to recovering eye position or the direction of attention.¹ The ssVEP-based BCIs may potentially be unpleasant for the users who have to attend the repetitive high-frequency (usually about 10 Hz) flashing visual stimuli for the BCI to generate continuous outputs.

The objective of this paper is, therefore, to introduce a high-performance BCI methodology based on steady-state finger-movement related potentials, independent of eye direction. In this approach, low-frequency (2 Hz) flashing visual stimuli are exploited, and the subjects are asked to tap in synchrony with them rather than to gaze at them. It has been shown [1] that RPs of about 2 Hz are EEG correlates of voluntary movement preparation. Therefore, as a prime candidate, we used this frequency. Repp [20] in his extensive behavioral experiments has shown that sensorimotor synchronization to visual cues of up to maximum 3 Hz is possible. However, when audio signals are used, the synchronization may be maintained up to relatively higher frequencies of 7–8 Hz. However, in the BCI context, it is fair to say that the ssMRPs do not have the broad frequency range of ssVEPs, and whether EEG potentials generated by tapping with higher frequencies would be classifiable on the single-trial basis is subject to further research.

¹Recently, Kelly *et al.* [19] have reported an ssVEP-based BCI independent from gaze direction by classification of VEPs recorded during visual spatial attention.

Execution of simple unimanual repetitive finger movements is associated with activity within the Rolandic fissure of the contralateral hemisphere corresponding to the primary sensorimotor cortex [21]. Our behavioral neuroimaging studies on rhythmic movements have led to the hypothesis that there are distinct brain structures that perform *automatic* versus *cognitively controlled* (CC) timing for repetitive movements [22], [23]. The automatic control (AC) system is primarily involved in continuous movements with frequencies greater than 1 Hz, i.e., subsecond intervals. It is likely to employ neural assemblies within the primary motor system. Furthermore, we have concluded that once a fast rhythmic task is selected and initiated, it may be executed without direct attention [24]. The timing control of a continuous series of fast and predictable movements should therefore require attention merely during the selection and initiation phases. On the other hand, the CC timing system is more exploited in controlling movements at intervals much longer than 1 s, i.e., at <1 Hz frequencies. The CC timing structure requires the activation of additional lateralized prefrontal and parietal lobe structures.

Schaal *et al.* [25] have verified that in discrete single-joint movements, higher brain functions such as working memory (the dorsolateral prefrontal cortex), recall (the ventrolateral prefrontal cortex), and attention (the intraparietal sulcus and inferior parietal lobe) may be involved. In contrast, rhythmic movements show much less cerebral activity; the only significantly active region is the contralateral motor cortex. Intuitively, one would assign the AC system for timing of rhythmic movements and the CC systems for discrete movements.

Conventionally, in BCI, subjects are instructed to move (imagine the movement of) their finger on a discrete-time basis. In contrast, it is hypothesized here that during fast rhythmic finger tapping, the AC timing system is involved, and hence, ssMRPs are confined to the contralateral sensorimotor cortex. This, in turn, implies that nonrhythmic motor-related activities emanating from frontal cortex will be attenuated. Therefore, if a motor task is carried out (real or imaginary) synchronized to a rhythmic (2 Hz) stimulus, the neural responses (ssMRPs) will oscillate at the same frequency, and hence, there should be a peak in the power spectrum of the recorded EEGs at the frequency of the oscillatory cue (and possibly its harmonics). Interestingly, this peak can represent a carrier frequency by which the EEGs are modulated. If the oscillations show stronger amplitudes on the hemisphere contralateral to the moving finger, the ssMRP can be regarded as a potential signal for BCI applications.

III. METHOD

Two experiments were conducted to test the ssMRP-based BCI in practice. First, we recorded ssMRPs during repetitive *real* finger movements. In the second experiment, we further investigated the potential and limitations of the ssMRPs-based BCI. Specifically, we address the following three issues. First, we document the transient effect of the visually evoked potentials (VEPs) caused by repetitive visual stimuli on the proposed BCI system. Second, we discuss how the proposed method is extensible to imagined movements. The classification scores of




Fig. 1. Temporal structure of each trial; first dataset.

EEGs recorded during imagined rhythmic movement are presented following a short overview of the rhythmic modulation of cortical potentials by imagined tapping. Third, repetition of a movement at an exact pace usually relies on an external stimulus—at least in the initiation and synchronization stages. This limitation can constrain the “real-life” applicability of the ssMRP-based BCI machines. We, therefore, recorded ssMRPs but without presenting the visual cues to objectively investigate to what extent a learned pace can be maintained. EEG analysis, i.e., preprocessing and classification, in these two scenarios is the same as those addressed in experiment I.

A. Experiment 1: Real Movements

Five right-handed healthy individuals (one female) (age 33 ± 9) participated in the first experiment. They had normal or corrected-to-normal vision, with no apparent motor problems and no previous BCI experience. All gave informed consent. Subjects I and III had previous musical training.

In this experiment, EEG signals were recorded during rhythmic left or right finger tapping. The experiment was run in a quiet, normally illuminated room. The participants were seated comfortably in an armchair with the forearms placed on the armrests of the chair. Two force transducers were attached to the armrests, on top of which the participants held their index fingers of each hand. The stimuli were presented in white against a gray background on a 17-in monitor at a resolution of 800×600 . The viewing distance was set to 100 cm.

The Ag/AgCl scalp electrodes were placed according to the 10-5 system [26] using a carefully positioned nylon cap. The EEG potentials were recorded continuously with 128 electrodes relative to an (offline) averaged left and right mastoid reference. The eye movements and blinks were monitored by bipolar horizontal and vertical electrooculogram (EOG) derivations. The EEG and EOG signals were amplified with a bandpass of 0–128 Hz using a BioSemi Active-Two amplifier and sampled at 512 Hz.

Each of five subjects first underwent a practice block of 20 trials. The main recording session comprised of eight blocks, each containing 40 trials, thus resulting in 320 trials for further analysis. The trial temporal structure is illustrated in Fig. 1. Each trial lasted 7 s, which included 1 s for initial fixation and another 6 s for EEG recording during rhythmic tapping. In the first second of each trial, a fixation cross “+” was shown in the center of the screen. Subsequently, while the cross was kept constant in the center, two rhythmically flashing “X”s appeared at the left and right sides of the cross for 6 s; each was 10 cm away from the center. The flashing frequency was set to 2 Hz. The participants were instructed to tap on one of the force sensors




Fig. 2. Temporal structure of each trial; second dataset.

under left or right index finger at a constant rate of 2 Hz in time with the flashing cues. The rest interval between trials was approximately 1.5 s, randomly changing with a variance of 150 ms, so that the subjects would not guess the start of next trial. The choice between right and left finger tapping was made freely by the participants in each trial. However, they were asked to be fair between right and left responses. Therefore, on average, we collected almost equal number of trials in each class across subjects.

The main reason for showing the flashing cues was to give the subjects a 2-Hz pace. Equidistant visual cues on either side from the center should not cause asymmetrically distributed potentials over the motor cortex. Moreover, the subjects were asked to maintain fixation on the central cross during the course of tapping. Later, in Section IV-D, we show how eye fixation and inattention to the cues should attenuate the stimulus-driven VEPs. Force transducers were utilized instead of conventional response switches in order to provide a setup in which the subjects did not actually press any switch, just performed repetitive tapping, which maintained the continuity of the repetitive finger movement.

B. Experiment 2: Imaginary Movements

In this experiment, we investigated the ssMRPs generated during imaginary movements. One right-handed healthy male (age 32) who did not have any BCI experience took part in this study; he had not participated in the first experiment. The EEG recording hardware setup was as described earlier in Section III-A. The recording session was comprised of eight blocks, each containing 30 trials, thus resulting in 240 trials for further analysis; almost equal number of trials for left and right fingers were recorded. This subject also first underwent a practice block of 20 trials.

The trial temporal structure is illustrated in Fig. 2. Each trial lasted 12 s, which included 2 s for initial fixation and 2 s for synchronizing the correct 2 Hz pace with the visual cues. Next followed a 3-s period when imagined rhythmic finger movements were carried out. Next came another 3 s period when the subject was instructed to make real tapping movement, but without the rhythmic visual cues on the screen. In the final 2 s, the visual cues reappeared on the screen to give a feedback on synchronization. The subject was asked to continue tapping in time with the cues; the data recorded in the last period was not analyzed. Throughout the 12 s, the fixation cross was maintained in the middle of the screen, and the participant was asked to maintain fixation throughout the trial. Note that the switching time between the third stage (imagination of movement) and the fourth stage (real tapping without cue) was instructed to the

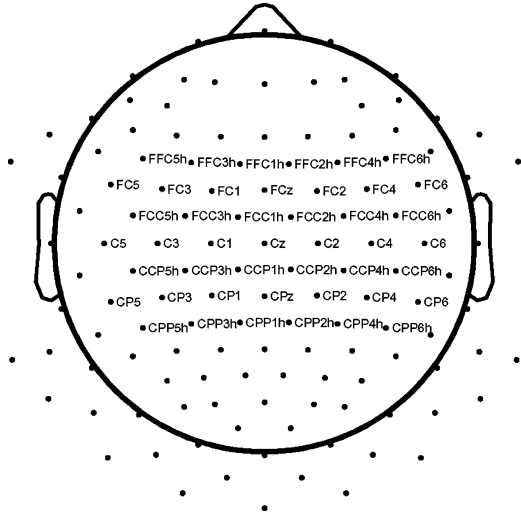


Fig. 3. Forty-five electrodes over the sensorimotor cortex that were included in the classification.

subject by replacing the central fixation cross “+” with an “X” for 100 ms.

C. Preprocessing

The EEG preprocessing was performed offline using BrainVision Analyzer (Brain Products GmbH). Continuous EEG recordings were offline segmented in epochs from 1 to 7 s after the trial onset in the first and 2 to 10 s in the second set of measurements. Specifically, we followed a dual-stage artifact rejection procedure: first, all trials in which the absolute difference between the maximum and minimum values of each vertical EOG channel was greater than $100 \mu\text{V}$ were rejected. Then, we visually searched and rejected the trials in which other artifacts, e.g., body/eye movements or electrode displacements, were evident.

On average, 15% and 10% of trials were rejected in the first and second experiments, respectively. Multichannel EEG measurements from scalp electrodes were then narrow bandpass filtered between 1.5 and 2.5 Hz. The preprocessed EEG segments, on average, almost equal to the number of trials in each class per subject, were exported to MATLAB for the single-trial feature extraction and classification stages.

D. Feature Extraction

Preprocessed trials from 45 electrode signals over the sensorimotor cortex area were considered; Fig. 3 depicts these electrodes. Each trial was temporally subsegmented into several overlapping windows. The energies of the bandpassed EEG recordings were computed in each data window, and the feature vectors were constructed. The energy features are approximately chi-square distributed, and therefore, taking the logarithm makes them almost Gaussian distributed, and a linear second-order statistics-based classifier such as Fisher’s linear discriminant (FLD) (see Section III-E) is expected to perform better [27]. Therefore, the classification operations were repeated using the log-energy features of EEGs. The left and right finger movement

classification was performed after the feature space dimension reduction using principal component analysis (PCA).

In a further step, in order to accentuate the localized activity and reduce volume conduction effects in multichannel EEG, the current source density (CSD) transform (available in the BrainVision Analyzer software) was used before computing the features of preprocessed signals. We expect that implementation of the CSD before the feature extracting stage would increase the classifier performance.

E. Classifier Design

The linear discriminant analysis (LDA) classifier based on the Fisher’s ratio [28] is utilized here mainly due to its simple computations. For a two-class classification problem, assume that the training patterns is given as $\mathcal{X} = \{\mathbf{x}_1, \mathbf{x}_2, \dots, \mathbf{x}_l\} = \{\mathcal{X}_1, \mathcal{X}_2\} \subset \mathbb{R}^N$, where the elements of $\mathcal{X}_1 = \{\mathbf{x}_1^1, \mathbf{x}_2^1, \dots, \mathbf{x}_{l_1}^1\}$ belong to class \mathcal{L}_1 , and similarly, $\mathcal{X}_2 = \{\mathbf{x}_1^2, \mathbf{x}_2^2, \dots, \mathbf{x}_{l_2}^2\}$ contains patterns from \mathcal{L}_2 . The FLD computes a vector \mathbf{w} to maximize the between-class distance while minimizing the within-class distance of the feature samples by a linear mapping as $f(\mathbf{x}) = \langle \mathbf{w} \cdot \mathbf{x} \rangle + b$, where $\langle \cdot \rangle$ denotes inner product operator. Vector \mathbf{w} may be computed by maximizing the class separability criterion $J(\mathbf{w})$

$$\mathbf{w} = \max_{\mathbf{w}} J(\mathbf{w}) = \max_{\mathbf{w}} \frac{\mathbf{w}' \mathbf{S}_B \mathbf{w}}{\mathbf{w}' \mathbf{S}_W \mathbf{w}} \quad (1)$$

where \mathbf{S}_B and \mathbf{S}_W are, respectively, the between- and within-class scatter matrices. The bias b of the linear rule is determined using $\langle \mathbf{w} \cdot \mathbf{m}_1 \rangle + b = -(\langle \mathbf{w} \cdot \mathbf{m}_2 \rangle + b)$, and the solution to (1) is $\mathbf{w} = \mathbf{S}_W^{-1}(\mathbf{m}_1 - \mathbf{m}_2)$ [28].

IV. RESULTS

The results of each experiment are reported separately here. For Experiment 1 the averaged ssMRPs are presented first. We subsequently report the results of our BCI scheme during the movement initiation and the synchronization states and also during the course of the trials. The effect of the time window size on the BCI performance is then investigated in Section IV-C. We also report the effect of the coexisting transient VEPs on the ssMRP measurement, ssMRP extension to motor imagery BCI, and separability of ssMRP-based BCI generated without presenting the visual cues.

A. Topographic Analysis of the Averaged EEG Recordings

Of primary interest was the ssMRPs developed during rhythmic tapping. Therefore, bandpass filtered (1.5–2.5 Hz) and CSD [29] transformed EEGs recorded during repetitive left and right finger movement trials from the representative subject I were used to visualize the ssMRPs in the time domain. The respective topographic maps (see Figs. 4 and 5) show a rapid development of lateralized rhythmic activity over the contralateral sensorimotor cortex. Topographical maps show snapshots of the spatial distribution of the ssMRPs every 250 ms, i.e., at peaks and troughs of 2 Hz rhythm.




Fig. 4. Averaged preprocessed EEGs during repetitive left finger movement for subject I. Topographical maps have been depicted in consecutive 0.25 s TWs. The top-left map illustrates the averaged EEGs over 0 and 0.25 s TWs, and the bottom right ones present those of the last 0.25 s window, i.e., 5.75–6 s. Note the rapid development of the lateralized 2 Hz signal on the contralateral right hemisphere.

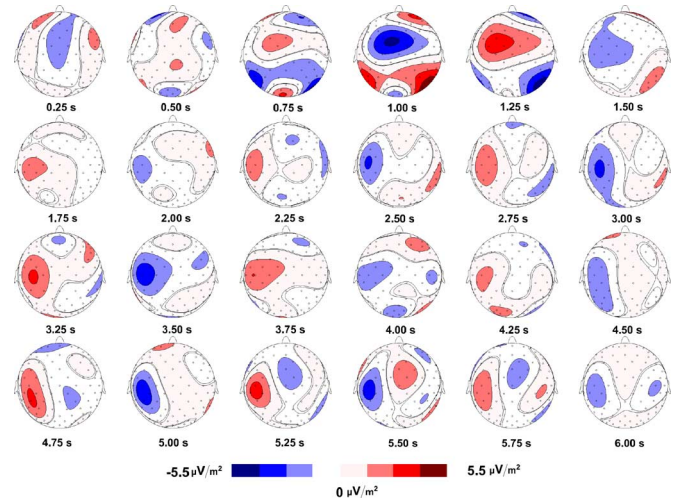


Fig. 5. Averaged preprocessed EEGs during repetitive right finger movement for subject I. Topographical maps have been depicted in consecutive 0.25 s TWs. The top-left map illustrates the averaged EEGs over 0 and 0.25 s TWs, and the bottom right ones present those of the last 0.25 s window, i.e., 5.75–6 s. Note the rapid development of the lateralized 2 Hz signal on the contralateral left hemisphere.

B. Classification During Initiation of Rhythmic Tapping

The experiment was designed in such a way that in the first second of each trial, the subjects initiated the rhythmic movement by adopting the correct 2 Hz pace from the visual cues, and then continued tapping with the acquired rhythm. Movement initiation may cause EEG activities coming from bilateral or lateralized areas of the brain other than the contralateral sensorimotor cortex, which can result in slight degradation in the BCI classification performance. Particularly, these activities may be attributed to potentials generated by frontal structures including presupplementary motor area (preSMA) and dorsal premotor cortex (dPMC), engaged during finger selection, movement initiation, and synchronizing to the external cue [24]. In addition, in order to tap in synchrony with the visual stimuli, attending to the visual cues inevitably causes VEPs to be produced by posterior visual areas. Therefore, one would expect that poor classification performance would be achieved during the selection and initiation phases in each trial. The performance should eventually increase after the first second.

In order to investigate how much EEG data should be recorded after the trial onset to have a reliable BCI output, we considered the eight first time intervals, i.e., 0–0.5, 0–1, 0–1.5, 0–2, 0–2.5, 0–3, 0–3.5, and 0–4 s. For classification, the 45 electrode signals over the sensorimotor cortex area depicted in Fig. 3 were considered. The feature vector consisted of the (logarithms of the) signal powers at 2 Hz in two conditions: with and without the CSD transform. In order to reduce the dimension of the classifier input space, we used PCA transform and introduced the first three principal components of the feature vectors to the FLD classifier. The classifier was trained on a randomly selected 60% of the resulting reduced feature vectors and tested with the remaining 40%. This cross validation pro-

cedure was repeated 400 times. The averaged classification results and their corresponding standard deviations are detailed in Tables I and II.

Note that the first two time intervals, 0–0.5 and 0–1 s, may be too short to include enough cycles of the 2 Hz rhythm to allow reliable BCI results. However, they can provide an indication of the lower bound of the classifier performance, which eventually increases in later intervals. Tables I and II report that the implementation of the CSD transform increased the CCR for subjects II, IV, and V. However, it did not enhance the performance for subjects I and III. Interestingly, for these two subjects, the classification results were in an acceptable range in the very early TWs, indicating that following initiation, synchronization stabilized very fast. This might be due to their previous musical training. All subjects had a short training block before the actual recording; nevertheless, they reported afterwards that they had to attend to the pace or the onset of each trial. As expected, Tables I and II report that higher classification results can be achieved if the log-energies of the EEGs are fed to the classifier.

C. Classification Through the Trial

After the initiation and the synchronization phases, subjects can keep tapping at almost the exact correct pace. Hence, one could predict that classification based on steady tapping, after the initiation, would be highly reliable. In order to test this finding in the BCI context, we classified the log-energy features of bandpass filtered EEGs in multiple overlapping TWs. Particularly, the discrimination accuracy was compared for three different sliding TW durations, i.e., $L = 1$ s, $L = 2$ s, and $L = 3$ s, and the sliding step was set to 0.125 s. Therefore, for $L = 1$, the TWs were 0–1, 0.125–1.125, ..., and 5–6 s, for $L = 2$, they were as 0–2, 0.125–2.25, ..., and 4–6 s, and likewise, for

TABLE I
AVERAGED CCRs AND THEIR CORRESPONDING STANDARD DEVIATIONS IN PERCENT DURING MOVEMENT INITIATION; WITHOUT CSD

Interval vs. Subject	I		II		III		IV		V	
Feature →	E	log(E)	E	log(E)	E	log(E)	E	log(E)	E	log(E)
0 - 0.5 s	78.16 ± 5.3	80.36 ± 4.8	76.37 ± 3.8	76.69 ± 3.8	90.17 ± 2.8	99.40 ± 0.6	56.00 ± 3.1	58.54 ± 3.1	68.94 ± 2.7	59.45 ± 3.1
0 - 1 s	84.79 ± 5.0	88.78 ± 4.0	76.49 ± 3.4	79.16 ± 3.7	97.60 ± 1.5	99.39 ± 0.5	56.65 ± 4.0	80.71 ± 2.9	77.63 ± 2.3	75.96 ± 2.2
0 - 1.5 s	87.46 ± 4.1	88.93 ± 3.6	80.39 ± 3.5	79.60 ± 3.4	95.72 ± 1.8	99.44 ± 0.6	60.58 ± 3.1	86.82 ± 2.1	78.72 ± 2.2	78.59 ± 2.1
0 - 2 s	93.93 ± 2.8	97.75 ± 2.7	70.78 ± 3.9	95.92 ± 2.1	97.43 ± 1.3	99.82 ± 0.3	60.79 ± 3.5	95.75 ± 1.4	82.70 ± 2.1	83.59 ± 1.8
0 - 2.5 s	94.98 ± 2.8	94.48 ± 2.7	69.83 ± 4.2	97.79 ± 1.2	97.63 ± 1.3	100.00 ± 0.0	56.46 ± 3.3	98.49 ± 0.7	83.98 ± 2.0	83.22 ± 2.1
0 - 3 s	93.80 ± 3.1	94.89 ± 2.6	82.36 ± 3.4	97.23 ± 1.5	99.29 ± 0.0	99.93 ± 0.1	50.44 ± 4.2	99.18 ± 0.4	83.24 ± 2.2	80.12 ± 2.2
0 - 3.5 s	91.63 ± 3.4	94.26 ± 1.4	80.44 ± 3.3	85.18 ± 3.2	98.78 ± 0.9	100.00 ± 0.0	75.06 ± 2.6	99.54 ± 0.4	78.68 ± 2.6	80.00 ± 2.2
0 - 4 s	91.61 ± 3.7	99.28 ± 0.9	76.04 ± 3.9	83.38 ± 3.1	98.94 ± 0.9	100.00 ± 0.0	85.86 ± 2.2	99.61 ± 0.3	79.29 ± 2.3	81.11 ± 2.2
Average	89.54	92.34	76.58	86.86	96.94	99.74	62.73	89.83	79.14	77.75

TABLE II
AVERAGED CCR AND THEIR CORRESPONDING STANDARD DEVIATIONS IN PERCENT DURING MOVEMENT INITIATION; WITH CSD

Interval vs. Subject	I		II		III		IV		V	
Feature →	E	log(E)	E	log(E)	E	log(E)	E	log(E)	E	log(E)
0 - 0.5 s	85.03 ± 3.6	92.61 ± 2.4	73.18 ± 3.7	79.56 ± 3.1	87.14 ± 2.8	96.56 ± 1.5	54.46 ± 3.7	66.84 ± 3.1	65.28 ± 2.4	83.52 ± 2.0
0 - 1 s	87.51 ± 3.0	89.24 ± 2.5	78.05 ± 3.9	81.64 ± 2.8	92.98 ± 2.2	98.81 ± 0.9	91.48 ± 1.2	96.84 ± 1.2	93.55 ± 2.5	99.21 ± 0.2
0 - 1.5 s	78.10 ± 3.7	95.73 ± 1.7	80.14 ± 3.3	94.87 ± 1.7	93.53 ± 2.2	99.98 ± 0.0	95.11 ± 1.7	99.44 ± 0.2	95.18 ± 1.6	99.67 ± 0.0
0 - 2 s	85.00 ± 3.3	98.22 ± 1.1	95.39 ± 1.3	99.33 ± 0.7	96.64 ± 1.2	100.00 ± 0.0	91.62 ± 1.7	99.22 ± 0.2	95.62 ± 1.8	99.56 ± 0.0
0 - 2.5 s	87.74 ± 3.2	98.73 ± 0.9	92.59 ± 2.2	98.19 ± 1.2	97.80 ± 1.3	100.00 ± 0.0	89.68 ± 1.8	99.16 ± 0.7	97.40 ± 1.2	99.30 ± 0.1
0 - 3 s	89.88 ± 0.1	98.18 ± 1.1	94.55 ± 2.1	97.26 ± 1.4	98.51 ± 0.9	99.93 ± 0.1	90.75 ± 1.8	99.60 ± 0.1	97.61 ± 0.9	98.81 ± 0.6
0 - 3.5 s	91.74 ± 2.6	98.11 ± 1.0	93.60 ± 2.0	96.50 ± 2.1	99.07 ± 0.8	100.00 ± 0.0	93.38 ± 2.2	99.26 ± 0.2	98.92 ± 0.2	99.22 ± 0.2
0 - 4 s	95.29 ± 1.8	98.80 ± 1.1	98.99 ± 0.7	99.36 ± 0.3	99.50 ± 0.4	100.00 ± 0.0	93.14 ± 1.7	95.51 ± 0.4	98.74 ± 1.7	99.42 ± 0.2
Average	87.53	96.20	88.31	93.36	95.64	99.41	87.45	94.48	92.78	97.33

TABLE III
AVERAGED CCRs, THEIR CORRESPONDING STANDARD DEVIATIONS IN PERCENT, AND AVERAGED ITRs IN BPM AND THE EFFECT OF TW SIZE; WITHOUT CSD

Subject	I		II		III		IV		V		Average	
TW	CCR	ITR	CCR	ITR	CCR	ITR	CCR	ITR	CCR	ITR	CCR	
1 s	Min	53.93 ± 5.0	0.2	49.93 ± 4.8	0.0	87.94 ± 7.9	28.1	55.28 ± 3.6	0.4	81.72 ± 3.9	18.8	86.09
	Avg	89.21 ± 9.4	30.3	71.70 ± 12.5	8.4	98.50 ± 2.2	53.2	76.01 ± 9.6	12.3	95.03 ± 5.1	42.8	
	Max	98.77 ± 1.4	54.2	99.43 ± 0.7	57.0	99.93 ± 0.0	59.5	95.62 ± 1.3	44.3	99.96 ± 0.0	58.0	
2 s	Min	78.57 ± 4.2	7.5	59.39 ± 4.5	0.7	98.75 ± 0.9	27.0	66.43 ± 3.1	2.3	88.83 ± 2.8	14.8	91.20
	Avg	93.42 ± 5.3	19.5	81.32 ± 10.5	9.1	99.50 ± 0.3	28.6	83.48 ± 9.4	10.6	98.28 ± 2.8	26.2	
	Max	99.52 ± 0.7	28.6	99.62 ± 0.5	28.9	100.00 ± 0.0	30.0	99.05 ± 0.6	27.7	99.69 ± 0.0	29.0	
3 s	Min	88.84 ± 3.2	9.9	68.02 ± 4.6	1.9	98.95 ± 0.7	18.3	76.20 ± 2.8	4.1	99.25 ± 0.1	18.7	93.55
	Avg	96.94 ± 2.9	16.0	82.10 ± 7.6	6.4	99.72 ± 0.3	19.4	89.54 ± 7.5	10.3	99.49 ± 0.1	19.0	
	Max	99.97 ± 0.1	19.9	94.93 ± 1.7	14.2	100.00 ± 0.0	20.0	99.61 ± 0.3	19.2	99.68 ± 0.0	19.3	

$L = 3$, the windows 0–3, 0.125–3.125, . . . , and 3–6 s were considered. Moreover, the ITR (in bpm) as the second measure of performance was computed for each TW size according to [13] as

$$\text{ITR (in bpm)} = \left[\log_2 N + P \log_2 P + (1 - P) \log_2 \frac{1 - P}{N - 1} \right] \times \frac{60}{L} \quad (2)$$

where $N = 2$ is the number of classes, P is the probability of correct classification, and L is the length of the window in seconds.

The same 45 electrode signals over the sensorimotor cortex area were considered. For each window size, we randomly selected 60% of the computed log-energy feature vectors for FLD training and the remaining 40% of the feature vectors were used for FLD testing. The random selection and classification procedures were repeated 400 times. We experimentally

concluded that the first three principal components of the feature space yield acceptable CCRs for our dataset. Evidently, more advanced pattern classification and dimensionality reduction techniques can be utilized for performance optimization, which fall outside the scope of this paper. Tables III and IV summarize the achieved performances. For each TW size and for each subject, the minimum and maximum computed CCRs and ITRs are also reported.

As expected, in both Tables III and IV for all five subjects, the averaged CCRs increase when larger TWs are considered. On the other hand, the ITR is inherently influenced by the decision speed, i.e., the length of the TW L ; the averaged ITRs decrease when L increases. Therefore, as for any other BCI mechanism, in ssMRP-based BCI, there is a tradeoff between the feature extraction window size and the BCI speed. The utilization of the CSD transform and the logarithm of energy as feature resulted in apparent higher averaged CCRs in Table IV compared to Table III.

TABLE IV
AVERAGED CCRs, THEIR CORRESPONDING STANDARD DEVIATIONS IN PERCENT, AND AVERAGED ITRs IN BPM AND THE EFFECT OF TW SIZE; WITH CSD

Subject		I		II		III		IV		V		Average
TW		CCR	ITR	CCR	ITR	CCR	ITR	CCR	ITR	CCR	ITR	CCR
1 s	Min	56.86 ± 3.5	0.8	65.70 ± 4.2	4.3	95.35 ± 3.8	43.7	74.78 ± 6.9	11.1	76.00 ± 4.6	12.3	89.71
	Avg	70.28 ± 13.0	7.3	93.28 ± 7.7	38.6	98.63 ± 0.9	53.7	89.73 ± 7.5	31.3	96.63 ± 4.4	47.2	
	Max	90.46 ± 2.2	32.7	99.60 ± 0.5	57.7	99.74 ± 0.2	58.4	99.52 ± 0.1	57.4	100.00 ± 0.0	60.0	
2 s	Min	50.99 ± 4.4	0.0	79.95 ± 3.9	8.3	97.99 ± 1.5	25.7	82.28 ± 5.4	9.7	94.85 ± 3.1	21.2	94.64
	Avg	82.61 ± 3.2	10.0	97.46 ± 3.8	24.8	99.23 ± 0.6	28.0	94.98 ± 5.1	21.3	98.93 ± 1.0	27.4	
	Max	93.50 ± 2.1	19.6	99.63 ± 0.5	28.9	100.00 ± 0.0	30.0	99.49 ± 0.2	28.5	100.00 ± 0.0	30.0	
3 s	Min	71.40 ± 4.0	2.7	86.39 ± 3.3	8.5	98.81 ± 0.8	18.1	94.63 ± 1.4	13.9	98.14 ± 0.4	17.3	95.99
	Avg	85.56 ± 6.8	8.0	97.74 ± 3.0	16.8	99.66 ± 0.4	19.3	98.03 ± 1.5	17.2	99.00 ± 0.2	18.3	
	Max	94.46 ± 2.1	13.8	99.64 ± 0.5	19.3	100.0 ± 0.0	20.0	99.63 ± 0.1	19.3	99.52 ± 0.1	19.1	

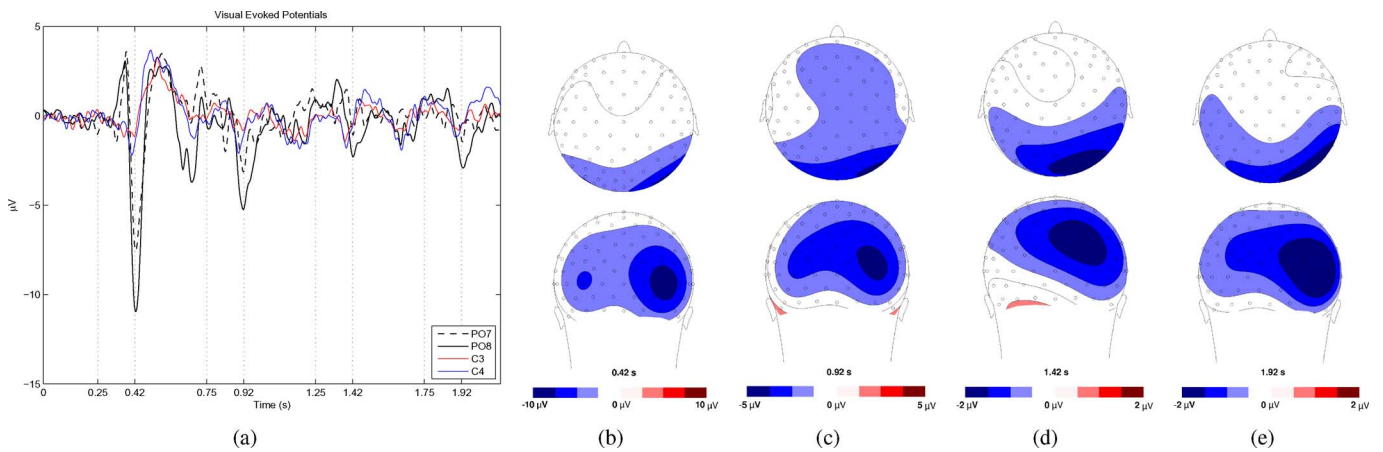


Fig. 6. Spatiotemporal patterns of VEPs recorded during the first 4 s of each trails. (a) Averaged VEPs from four representative electrodes in time. (b) Topographical distribution of first VEP at 0.42 ms, which is approximately 0.17 ms after the first visual cue. (c)–(e) Topographical distributions of the subsequent VEPs. Note the change in amplitude scaling of the topographic maps in (b)–(e).

D. Transient VEPs

Brain mechanisms of visual selective attention have been extensively explored by means of VEPs [30]. The VEP is elicited from the extrastriate visual cortex 80–200 ms after a stimulus is presented in an attended location within the subject’s visual field [30]. It has been verified [30], [31] that attention to the location where the visual stimulus appears enhances the sensory information and amplifies the consequent VEP.

In the context of our BCI protocol, we instructed the subject to fixate on the central cross, and not on the lateralized visual pacing cues. This approach attenuates the VEPs considerably. In Section IV-B, we mentioned that the subjects of the first experiment reported that they had to attend the visual cues at the beginning of each trial, which could lead to VEPs that lowered the classification performance in the first second of each trial (see Tables I and II).

In order to verify the correspondence between the attenuation of the VEPs and gradually improving CCRs, we monitored VEPs during the first 2 s of each trial (see Fig. 4). In that 2 s period, four visual stimuli were presented to the subject, and each was followed by a VEP after approximately 170 ms. Fig. 6(a) depicts the averaged VEPs across the period for electrode PO7, PO8, C3, and C4. The corresponding full-scale topographical distributions at times 0.42, 0.92, 1.42, and 1.92 s are plotted in

Fig. 6(b)–(e). Importantly, note the large amplitude of the first VEP and the attenuation of the following VEPs at PO8. This rapid attenuation would greatly reduce VEP contamination of ssMRPs after the first second. Moreover, either in the absence of or during a motor act the VEPs are largely confined to the visual cortex [see Fig. 6(b)–(e)]. Therefore, for BCI, VEP contamination of ssMRPs recorded from the motor cortex should be limited to only the beginning of each trial.

E. Imagination of Rhythmic Tapping for BCI

Cortical signals produced during overt or covert movements present similar spatiotemporal patterns as the motor cortex behaves in similar ways during both. It was shown in [32] that rhythmic imagination of left and right finger movements with frequencies greater than 1 Hz modulates cortical potentials and leads to ssMRPs. However, in rhythmic motor imagination, it is not possible to objectively verify whether the subject could successfully maintain the correct pace. Osman *et al.* [32] showed that high-frequency rhythmic motor imagination can be carried out after extensive subject training in real rhythmic motor actions.

We tested whether classification of ssMRPs recorded during rhythmic finger movement imagination is feasible for BCI applications. Hence, in the second experiment, the subject was

TABLE V
AVERAGED CCRs, THEIR CORRESPONDING STANDARD DEVIATIONS IN PERCENT, AND AVERAGED ITRs IN BPM FOR THE SECOND DATASET

Period		Motor Imagery		Without Cue	
TW		CCR	ITR	CCR	ITR
1 s	Min	83.47 ± 7.2	21.1	63.16 ± 6.1	3.0
	Avg	90.21 ± 3.2	32.2	81.36 ± 7.1	9.1
	Max	91.56 ± 0.9	34.9	95.92 ± 2.6	45.2
2 s	Min	92.78 ± 1.1	18.7	72.38 ± 5.0	4.5
	Avg	93.49 ± 0.4	19.5	84.79 ± 8.7	23.1
	Max	95.12 ± 0.4	21.5	98.44 ± 2.9	26.5




Fig. 7. Distribution of ITIs (time between successive taps) without and with the visual cues. Error bars show the standard deviations.

instructed to repetitively imagine left or right finger movements after the early fixation period and adopting the correct pace after fixation at the beginning of each trial (see Fig. 2). The same classification procedure using two TWs of lengths 1 and 2 s was carried out. The averaged CCRs, their corresponding standard deviations, and the ITRs are shown in Table V. The relatively high classification rates of about 90.2% and 93.4%, respectively, when the TW was 1 or 2 s, demonstrate the applicability of the ssMRPs for motor-imagery-based BCI. Note that as in Section IV-C, using a wider TW enhances the classification performance, but reduces the ITR.

F. Extension to BCI Without Visual Cue

All established BCI approaches require external visual or audio cues to certain levels. For instance, the ssVEP- or P300-based BCI would not be possible without the visual stimuli. However, the ssMRPs can be generated without the visual cues after the subjects adopt the correct pace. As shown in Fig. 4, in the fourth part of each trial, the subject started to rhythmically tap but without the rhythmic visual cue. Then, the subject was asked to continue tapping in the fifth period for another 2 s when the cues appeared.

The participant's success at tapping with the correct rhythm is reflected in Fig. 7, which displays the time between successive taps (ITIs). The fourth and the fifth periods included six and

four taps, respectively, and hence, 5 and 3 s intervals. Fig. 7 reports that the subject maintained a pace of approximately 2.2 Hz. Moreover, these results match our earlier findings that once a fast rhythmic action is started, it can be carried out almost automatically [24].

As before, two different TWs of 1 and 2 s were considered, and the pattern classification procedure was implemented; the results are reported in Table V. Note that the averaged CCRs during the "tapping without cue" are relatively lower than that of "motor imagery." This can be explained as transition from motor imagination to real movement could activate brain areas other than sensorimotor cortex, and consequently, a transient drop in the CCRs. Another potential cause could be the replacement of the central fixation cross with an "X" for about 100 ms, which elicits a VEP. As we utilize no spatial filtering to attenuate the effect of this VEP, deterioration of the CCRs is inevitable.

V. CONCLUSION

The present study used the ssMRPs to provide a measure of sensorimotor cortex activation during rhythmic tapping and suggested a potential application for a real-time high-accuracy BCI. In this approach, the subjects were asked to cyclically move their left or right index finger at a predetermined frequency. Therefore, the lateralized and band-limited ssMRP was detected from the sensorimotor cortex. The main advantage of the ssMRP-based BCI over other approaches is its simple recording setup and straightforward computations. Comparing to BCI machines based on RPs, using the ssMRP for BCI would not be difficult for the subjects since in each trial, they are actively involved in the experiment, rather than waiting for several seconds before the exertion of a single discrete movement.

Here, the ssMRP-based BCI has been tested for six healthy subjects. However, its physiological background and simplicity of the recording setup support the repeatability of the experiments. In the first experiment, the maximum performance was attained for data windows lying in the middle of each trial, at approximately 3–4 s after the movement onset in each trial for all participants. For most subjects, reliable classification rates could be achieved with shorter data lengths, and the average CCR for a data window of only 2 s with (or without) the CSD transform was 94.6% (or 91.2%).

The use of CSD transform and the log-energy features increased the performance. However, in order to test whether that increase is statistically significant, more subjects are needed. On the other hand, real-time implementation of such nonlinear transformation is not trivial. A simpler approach would be to incorporate the Laplacian derivative of EEGs at each electrode site, which is the second derivative of the spline function at that location. Similar to the CSD transform, it is related to the rate of change over space and amplifies the contribution of nearby electrical sources and diminishes that of distant ones.

We argue that the ssMRP-based BCI is simpler than the ssVEP-based BCI systems in terms of subject training time and signal analysis. In the proposed method, advanced spectral estimation algorithms are not necessary since instead of frequency separation of ssVEP, only one frequency is dealt with.

In other words, instead of exploiting the spectral disparity in the signal processing unit of the BCI machine, the topographical distribution of scalp EEG signals in the frequency band of interest is used to identify the effector. The ssMRP approach for BCI can be extended beyond the present example in a number of ways. To begin with, it should be possible to realize all the ssVEP-based applications by the ssMRPs where a continuous BCI signal rather than a chain of discrete outputs is needed; a prime example is robot or wheelchair navigation. Also, the large number of electrodes utilized in this research should not generally be regarded as a hindrance toward end-product BCI, and acceptable performance can be expected from fewer electrodes situated over the two motor cortices (see Fig. 5).

There is subtle difference here between our interpretation of the ssMRPs and that of Gerloff *et al.* [21], where each tap was treated individually for exploring EEG correlates of sensorimotor activity around the tap onset. However, in our research, we treat taps in a short train, i.e., in windows of 1, 2, or 3 s, and search for their EEG signatures. On the other hand, a challenging research question would be the classification of ssMRPs but on the classic tap-by-tap basis, which effectively follows [8] and [12]. It was shown in [21] that the averaged tap-by-tap segmented ssMRPs show distinct premovement motor and postmovement sensory components. For the premovement component, one would expect to identify a radial dipole source in the primary motor cortex contralateral to the side of the movement followed by a tangential postmovement source located in the primary sensory cortex slightly inferior to the former source. These two sources would reflect the repetitive efferent and reafferent motor outputs and sensory inputs. Therefore, capturing such a premovement EEG negative signatures of centroparietal activity followed by a complex of “frontal negative”-“parietal positive” EEG distribution can significantly enhance the performance of the ssMRP-based BCI if it can be realized for the single-trial data.

Note that there are also certain differences between our recording setup and those of previous studies such as [8] and [12] where the participants could alternate between right and left fingers in consecutive short intervals, i.e., the subject could decide whether to move the left or right index on each tap. The participants in [8] and [12] were not provided with rhythmic visual cues, and therefore, a series of discrete movements were carried out rather than rhythmic continuous movements. Therefore, as discussed in Section II, the lower classification performances they obtained might be due to the repetitive activation of the frontal cortex during the initiation of each discrete movement. The actual number of taps per hand and the interhand transition matrix in [8] had to be computed objectively and shown on the screen; the taps on the keyboard were extracted as markers into the stream of EEG measurements. Therefore, if the tap rate or the number of alterations deviated from preinstructed rate, the subject was informed so that these could be compensated accordingly. In such a scenario, one could not expect steady-state MRPs to be generated. Finally, in specific applications, such as typing on the keyboard, the BCI system should ideally be able to distinguish between left and right finger movements in each individual discrete tap. However, there are other applications

such as navigating a wheelchair, in which a smooth and continuous BCI output is demanded. We believe that with further refinements, our protocol will lead to a reliable and robust BCI.

ACKNOWLEDGMENT

The authors would like to acknowledge Dr. B. Blankertz at Berlin BCI for his comments on EEG recording protocol used in [8] and [12].

REFERENCES

- [1] M. Jahanshahi and M. Hallett, Eds., *The Bereitschaftspotential Movement Related Cortical Potentials*. Norwell, MA: Kluwer, 2003.
- [2] R. Q. Cui, D. Huter, W. Lang, and L. Deecke, “Neuroimage of voluntary movement: Topography of the Bereitschaftspotential, a 64-channel DC current source density study,” *NeuroImage*, vol. 9, pp. 124–134, 1999.
- [3] M. G. H. Coles, H. G. O. M. Smid, M. K. Scheffers, and L. J. Otten, “Electrophysiology of mind: Event-related brain potentials and cognition,” in *Mental Chronometry and the Study of Human Information Processing*, M. D. Rugg and M. G. H. Coles, Eds. Oxford, U.K.: Oxford Univ. Press, 1995, pp. 86–131.
- [4] P. Praamstra, D. F. Stegeman, A. R. Cools, and M. W. I. M. Horstink, “Reliance on external cues for movement initiation in Parkinson’s disease; evidence from movement related potentials,” *Brain*, vol. 121, pp. 167–177, 1998.
- [5] M. Kutas and E. Donchin, “Preparation to respond as manifested by movement related brain potentials,” *Brain Res.*, vol. 202, pp. 95–115, 1980.
- [6] M. G. H. Coles and G. Gratton, “Energetic and Human Information Processing,” in *Cognitive Psychophysiology and the Study of States and Processes*, G. R. J. Hockey, A. W. K. Gaillard, and M. G. H. Coles, Eds. Dordrecht, The Netherlands: Martinus Nijhoff, 1986, pp. 409–424.
- [7] T. Hinterberger, S. Schmidt, N. Neumann, J. Mellinger, B. Blankertz, G. Curio, and N. Birbaumer, “Brain–computer communication with slow cortical potentials,” *IEEE Trans. Biomed. Eng.*, vol. 51, no. 6, pp. 1011–1018, Jun. 2004.
- [8] B. Blankertz, G. Dornhege, M. Krauledat, K.-R. Müller, V. Kunzmann, F. Losch, and G. Curio, “The Berlin brain computer interface: EEG-based 2 communication without subject training,” *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 14, no. 2, pp. 147–152, Jun. 2006.
- [9] B. Blankertz, G. Dornhege, C. Schäfer, R. Krepki, K.-R. Müller, V. Kunzmann, F. Losch, and G. Curio, “Boosting bit rates and error detection for the classification of fast-paced motor commands based on single-trial EEG analysis,” *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 11, no. 2, pp. 127–131, Jun. 2003.
- [10] R. Krepki, B. Blankertz, G. Curio, and K.-R. Müller, “The Berlin brain–computer interface (BBCI)—Towards a new communication channel for online control in gaming applications,” *J. Multimedia Tools Appl.*, vol. 33, pp. 73–90, 2007.
- [11] R. Krepki, G. Curio, B. Blankertz, and K.-R. Müller, “Berlin brain–computer interface—The HCI communication channel for discovery,” *Int. J. Hum. Comput. Stud.*, vol. 65, pp. 460–477, 2007.
- [12] B. Blankertz, G. Dornhege, S. Lemm, M. Krauledat, G. Curio, and K.-R. Müller, “The Berlin brain–computer interface: Machine learning based detection of user specific brain states,” *J. Universal Comput. Sci.*, vol. 12, pp. 581–607, 2006.
- [13] J. R. Pierce, *An Introduction to Information Theory*. New York: Dover, 1980, pp. 145–165.
- [14] G. Dornhege, B. Blankertz, G. Curio, and K.-R. Müller, “Boosting bit rates in non-invasive EEG single-trial classifications by feature combination and multi-class paradigms,” *IEEE Trans. Biomed. Eng.*, vol. 51, no. 6, pp. 993–1002, Jun. 2004.
- [15] D. Regan, *Human Brain Electrophysiology: Evoked Potentials and Evoked Magnetic Fields in Science and Medicine*. Amsterdam, The Netherlands: Elsevier, 1989.
- [16] G. R. McMillan, G. L. Calhoun, M. S. Middendorf, J. H. Schnurer, D. F. Ingle, and V. T. Nasman, “Direct brain interface utilizing self-regulation of steady-state visual evoked response (SSVER),” in *Proc. RESNA*, Washington, DC, 1995, pp. 693–695.
- [17] G. R. Müller-Putz, R. Scherer, C. Brauneis, and G. Pfurtscheller, “Steady-state visual evoked potential (SSVEP)-based communication: Impact of harmonic frequency components,” *J. Neural Eng.*, vol. 2, pp. 123–130, 2005.

- [18] P. Martinez, H. Bakardjian, and A. Cichocki, "Fully online multicommand brain-computer interface with visual neurofeedback using SSVEP paradigm," *Comput. Intell. Neurosci.*, vol. 2007, pp. 94561-1-94561-9, 2007. DOI:10.1155/2007/94561.
- [19] S. P. Kelly, E. C. Lalor, R. B. Reilly, and J. J. Fox, "Visual spatial attention tracking using high-density SSVEP data for independent brain-computer communications," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 13, no. 2, pp. 172-178, Jun. 2005.
- [20] B. H. Repp, "Rate limits of sensorimotor synchronization," *Adv. Cogn. Psychol.*, vol. 2, pp. 163-181, 2006.
- [21] C. Gerloff, C. Toro, N. Uenishi, L. G. Cohen, L. Leocani, and M. Hallett, "Steady-state movement related cortical potentials: A new approach to assessing cortical activity associated with fast repetitive finger movements," *Electroencephalogr. Clin. Neurophysiol.*, vol. 102, pp. 106-113, 1997.
- [22] P. A. Lewis and R. C. Miall, "Distinct systems for automatic and cognitively controlled time measurement: Evidence from neuroimaging," *Curr. Opin. Neurobiol.*, vol. 13, pp. 250-255, 2003.
- [23] R. C. Miall and R. Ivry, "Moving to a different beat," *Nature Neurosci.*, vol. 7, no. 10, pp. 7-8, 2004.
- [24] P. A. Lewis, A. M. Wing, P. A. Pope, P. Pramstra, and R. C. Miall, "Brain activity correlates differentially with increasing temporal complexity of rhythms during selection, synchronisation, and continuation phases of paced finger tapping," *Neuropsychologia*, vol. 42, pp. 1301-1312, 2004.
- [25] S. Schaal, D. Sternad, R. Osu, and M. Kawato, "Rhythmic arm movement is not discrete," *Nature Neurosci.*, vol. 7, no. 10, pp. 1137-1144, 2004.
- [26] R. Oostenveld and P. Praamstra, "The five percent electrode system for high resolution EEG and ERP measurements," *Clin. Neurophysiol.*, vol. 112, pp. 713-719, 2001.
- [27] B. Blankertz, M. Kawanabe, R. Tomioka, F. Hohlefeld, V. Nikulin, and K.-R. Müller, "Invariant common spatial patterns: Alleviating nonstationarities in brain-computer interfacing," in *Proc. NIPS*, vol. 20, Cambridge, MA: MIT Press, 2008.
- [28] K. Fukunaga, *Introduction to Statistical Pattern Recognition*, 2nd ed. San Francisco, CA: Academic, 1990.
- [29] F. Perrin, J. Pernier, O. Bertrand, and J. Echallier, "Spherical splines for scalp potential and current density mapping," *Electroencephalogr. Clin. Neurophysiol.*, vol. 72, pp. 184-187, 1989.
- [30] M. I. Posner and S. Dehaene, "Attentional networks," *Trends Neurosci.*, vol. 17, no. 2, pp. 1643-1650, 1994.
- [31] S. T. Morgan, J. C. Hansen, and S. Hillyard, "Selective attention to stimulus location modulates the steady-state visual evoked potential," *Proc. Nat. Acad. Sci. USA*, vol. 93, pp. 4770-4774, 1996.
- [32] A. Osman, R. Albert, K. R. Ridderinkhof, G. Band, and M. van der Molen, "The beat goes on: Rhythmic modulation of cortical potentials by imagined tapping," *J. Exp. Psychol.: Hum. Perception Performance*, vol. 32, no. 4, pp. 986-1005, 2006.



Kianoush Nazarpour (S'05-M'09) received the B.Sc. degree in electrical engineering from KN Toosi University, of Technology, Tehran, Iran, in 2003, the M.Sc. degree in electrical engineering from Tarbiat Modarres University, Tehran, in 2005, and the Ph.D. degree in electrical engineering from Cardiff University, Cardiff, U.K., in 2008.

In 2007, he joined the School of Psychology, University of Birmingham, Birmingham, U.K., where he is currently a Research Fellow. His current research interests include the areas of biomedical signal processing and neuromuscular rehabilitation.

Dr. Nazarpour was the recipient of the Best Poster Award in the Third Brain-Computer Interface (BCI) Workshop, Graz, Austria, and the David Douglas Award from South Wales Institute of Engineers both in 2006 for his work on space-time-frequency (STF) decomposition of EEG potentials for BCI applications.



Peter Praamstra received the Ph.D. degree in medical sciences from Radboud University Nijmegen, Nijmegen, The Netherlands, in 1992.

He studied medicine in Nijmegen, where he was also trained in neurology and clinical neurophysiology. He is currently a Consultant Neurologist and a Reader in cognitive neurophysiology at the University of Birmingham, Birmingham, U.K. His current research interests include basal ganglia related movement disorders and motor neurophysiology related to response selection and preparation.



R. Chris Miall received the B.Sc. and Ph.D. degrees in zoology from Imperial College London, London, U.K.

In 2005, he joined the Behavioural Brain Sciences Centre, University of Birmingham, Birmingham, U.K., where he is currently a Professor of motor neuroscience. His current research interests include motor learning and motor coordination, usually in visually guided actions. His recent work has been directed toward questions of predictive knowledge and predictive control, and how these issues reflect on the use of "internal models" in the nervous system. He was engaged in research on tests of human motor psychophysics, with functional MRI and transcranial magnetic stimulation (TMS) as brain mapping techniques.

He was engaged in research on tests of human motor psychophysics, with functional MRI and transcranial magnetic stimulation (TMS) as brain mapping techniques.



Saeid Sanei (M'97-SM'05) received the Ph.D. degree from Imperial College of Science, Technology, and Medicine, London, U.K., in 1991.

He has been a member of the Academic Staff in Iran, Singapore, and U.K. He is currently a member of the Centre of Digital Signal Processing, Cardiff University, Cardiff, U.K. He has authored or coauthored more than 170 papers and a unique monogram in EEG signal processing. He is the Associate Editor of the *Journal of Computational Intelligence and Neuroscience*. His current research interests include

biomedical, acoustic, and communication signal processing, adaptive and nonlinear signal processing, and pattern recognition and classification.